


## H2S-B4 Hydrogen Sulfide Sensor – 4-Electrode

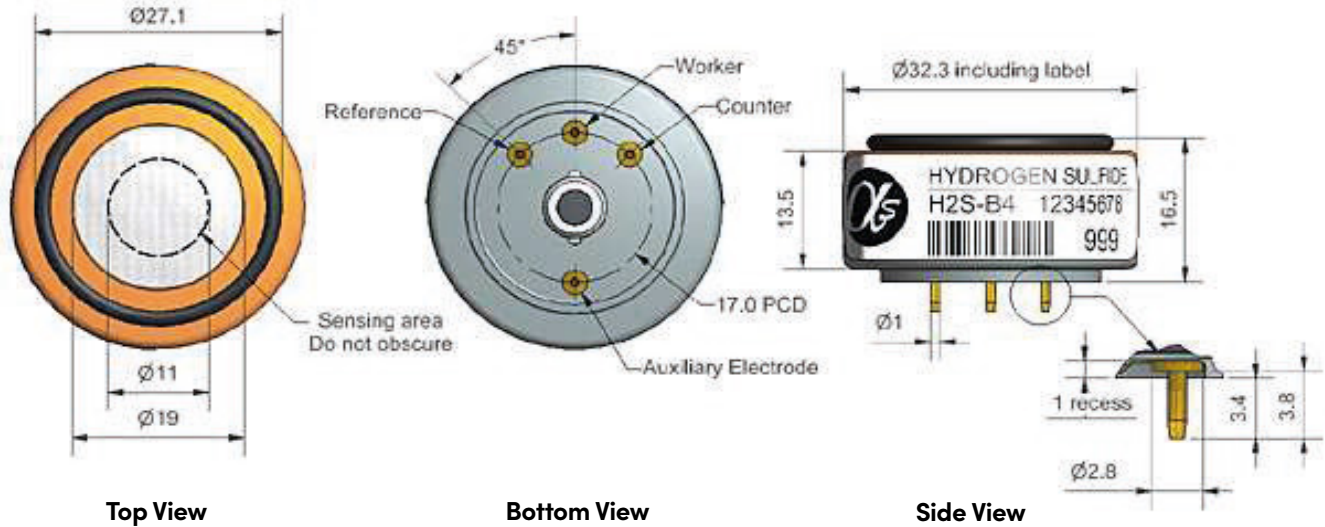

Dimensions are in millimetres ( $\pm 0.15$  mm).

### Performance

Sensitivity	nA/ppm at 2ppm H <sub>2</sub> S	1450 to 2600
Response time	t <sub>90</sub> (s) from zero to 2ppm H <sub>2</sub> S	< 60
Zero current	nA in zero air at 20°C	-250 to 200
Noise*	$\pm 2$ standard deviations (ppb equivalent)	1
Range	ppm H <sub>2</sub> S limit of performance warranty	100
Linearity	ppb error at full scale, linear at zero and 40ppm H <sub>2</sub> S	< $\pm 4$
Overgas limit	maximum ppm for stable response to gas pulse	200

\*Tested with Alphasense ISB low noise circuit

### Lifetime

Zero drift	ppm equivalent change/year in lab air	< $\pm 100$
Sensitivity drift	% change/year in lab air, monthly test	< 20
Operating life	months until 50% original signal (24-month warranted)	> 24

### Environmental

Sensitivity @ -20°C	% (output @ -20°C/output @ 20°C) @ 2ppm H <sub>2</sub> S	77 to 90
Sensitivity @ 50°C	% (output @ 50°C/output @ 20°C) @ 2ppm H <sub>2</sub> S	100 to 110
Zero @ -20°C	nA change from 20°C	50 to 60
Zero @ 50°C	nA change from 20°C	-120 to -160

### Cross Sensitivity

NO <sub>2</sub> sensitivity	% measured gas @ 5ppm	NO <sub>2</sub>	< -10
Cl <sub>2</sub> sensitivity	% measured gas @ 5ppm	Cl <sub>2</sub>	< -12
NO sensitivity	% measured gas @ 5ppm	NO	< 12
SO <sub>2</sub> sensitivity	% measured gas @ 5ppm	SO <sub>2</sub>	< 20
CO sensitivity	% measured gas @ 5ppm	CO	< 3
H <sub>2</sub> sensitivity	% measured gas @ 100ppm	H <sub>2</sub>	< 0.5
C <sub>2</sub> H <sub>4</sub> sensitivity	% measured gas @ 100ppm	C <sub>2</sub> H <sub>4</sub>	< 0.1
NH <sub>3</sub> sensitivity	% measured gas @ 20ppm	NH <sub>3</sub>	< 0.1
CO <sub>2</sub> sensitivity	% measured gas @ 5%	CO <sub>2</sub>	< 0.1

### Key Specifications

Temperature range	°C	-30 to 50
Pressure range	kPa	80 to 120
Humidity range	% rh continuous	15 to 90
Storage period	months @ 3 to 20°C (stored in sealed pot)	6
Load resistor	$\Omega$ (ISB circuit is recommended)	33 to 100
Weight	g	< 13

**Figure 1 Sensitivity Temperature Dependence**

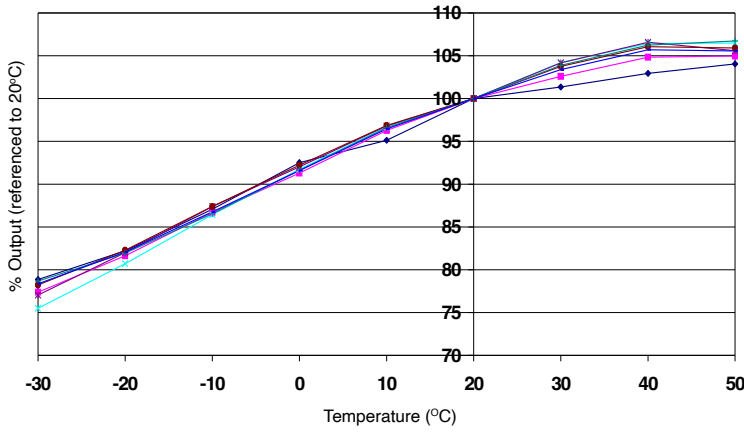


Figure 1 shows the temperature dependence of sensitivity at 2ppm H<sub>2</sub>S.  
This data is taken from a typical batch of sensors.

**Figure 2 Zero Temperature Dependence**

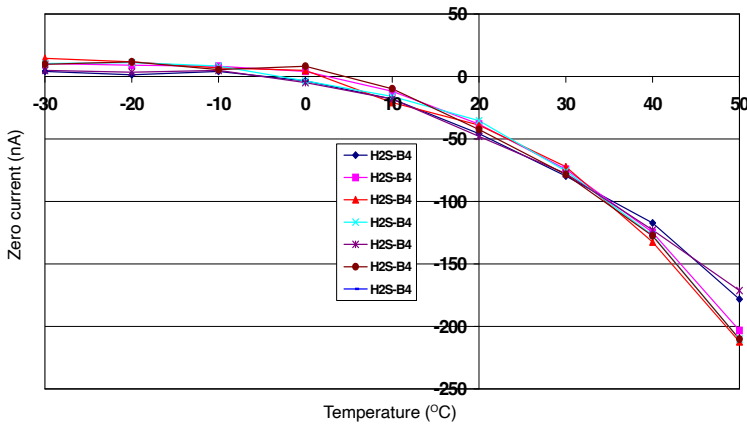


Figure 2 shows the variation in zero output of the working electrode caused by changes in temperature, expressed as nA.  
This data is taken from a typical batch of sensors.  
Contact Alphasense for further information on zero current correction.

**Figure 3 Linearity to 200 ppb H<sub>2</sub>S**

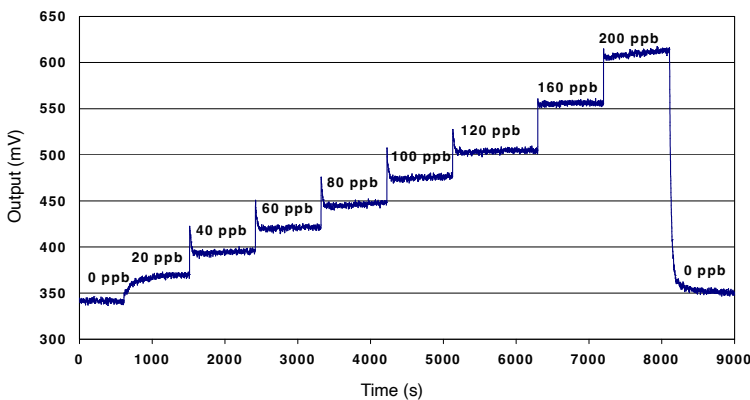


Figure 3 shows response to 200ppb H<sub>2</sub>S.  
Use of Alphasense ISB circuit reduces noise to 1ppb, with the opportunity of digital smoothing to reduce noise even further.

At the end of the product's life, do not dispose of any electronic sensor, component or instrument in the domestic waste, but contact the instrument manufacturer, Alphasense or its distributor for disposal instructions. NOTE: all sensors are tested at ambient environmental conditions unless otherwise stated. As applications of use are outside our control, the information provided is given without legal responsibility. Customers should test under their own conditions, to ensure that the sensors are suitable for their own requirements.

In the interest of continued product improvement, we reserve the right to change design features and specifications without prior notification. The data contained in this document is for guidance only. Alphasense Ltd accepts no liability for any consequential losses, injury or damage resulting from the use of this document or the information contained within. (©ALPHASENSE LTD) Doc. Ref. H2S-A4/OCT22